

ID No: 00411092023

TEST RESULT SHEET


Date 11 month 09 year 2023

1. SAMPLE INFORMATION:

Patient name: **KONG DANNY** Sex: **Female** Age: **28**
 Testing requirements: **HBV-DNA Quantitative**
 Address: **BIOKHON LAB**
 Test technique: **Real-time PCR – Photomultiplier Tube Technique**
The FAM labeled probe to detect the target DNA
The HEX labeled probe to detect the Internal control

2. RESULTS:

Amplification Plots

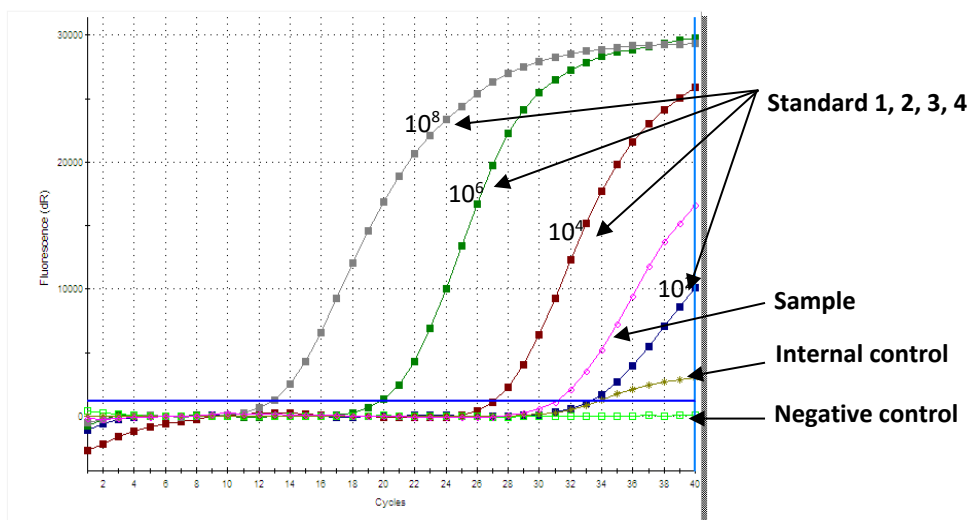

3. CONCLUSION:

The viral load: 4.39
 The viral load: 4,872
 The viral load: 24,362

\log_{10}
 IU/ml
 copies/ml

Limit of detection

$\leq 2.40 \log_{10}$
 $\leq 50 \text{ IU/mL}$
 $\leq 250 \text{ Copies/mL}$

CHARGE OF LAB



MA. NGUYEN THUY DA THAO