

ID No: 00410092023

TEST RESULT SHEET


Date 10 month 09 year 2023

1. SAMPLE INFORMATION:

Patient name: **NY VANNAK** Sex: **Male** Age: **42**
 Testing requirements: **HBV-DNA Quantitative**
 Address: **BIOKHON LAB**
 Test technique: **Real-time PCR – Photomultiplier Tube Technique**
The FAM labeled probe to detect the target DNA
The HEX labeled probe to detect the Internal control

2. RESULTS:

Amplification Plots

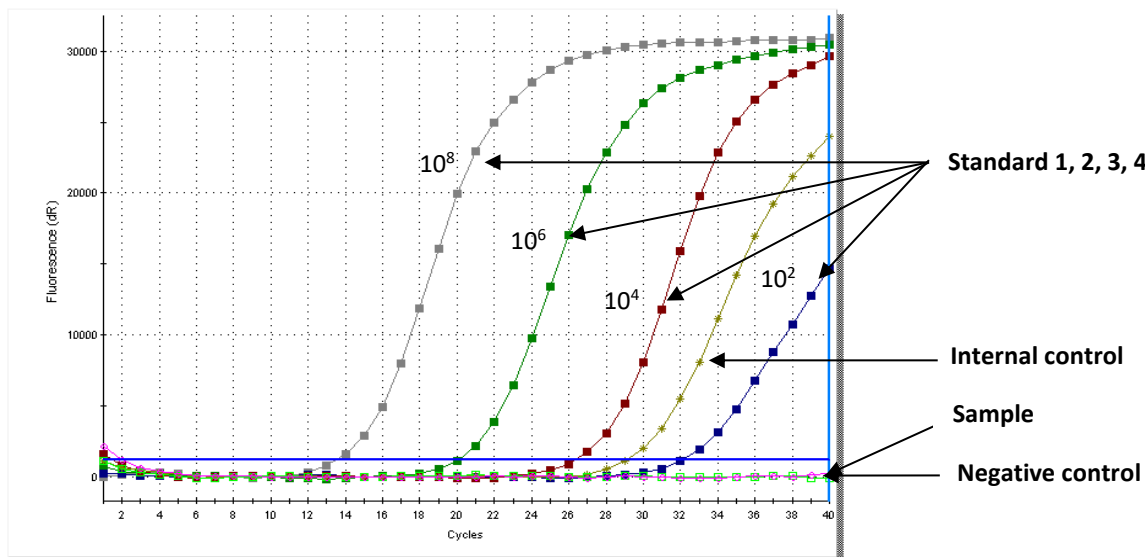

Threshold of quantitative: 250 copies/ml

Limit of detection

3. CONCLUSION:

Detected no virus in the sample.

$\leq 2.40 \log_{10}$

$\leq 50 \text{ IU/mL}$

$\leq 250 \text{ Copies/ml}$

CHARGE OF LAB



MA. NGUYEN THUY DA THAO