

ID No: 01317092023

TEST RESULT SHEET


Date 17 month 09 year 2023

1. SAMPLE INFORMATION:

Patient name: **CHHOUR LYKHEANG** Sex: **Male** Age: **78**
 Testing requirements: **HBV-DNA Quantitative**
 Address: **BIOKHON LAB**
 Test technique: **Real-time PCR – Photomultiplier Tube Technique**
The FAM labeled probe to detect the target DNA
The HEX labeled probe to detect the Internal control

2. RESULTS:

Amplification Plots

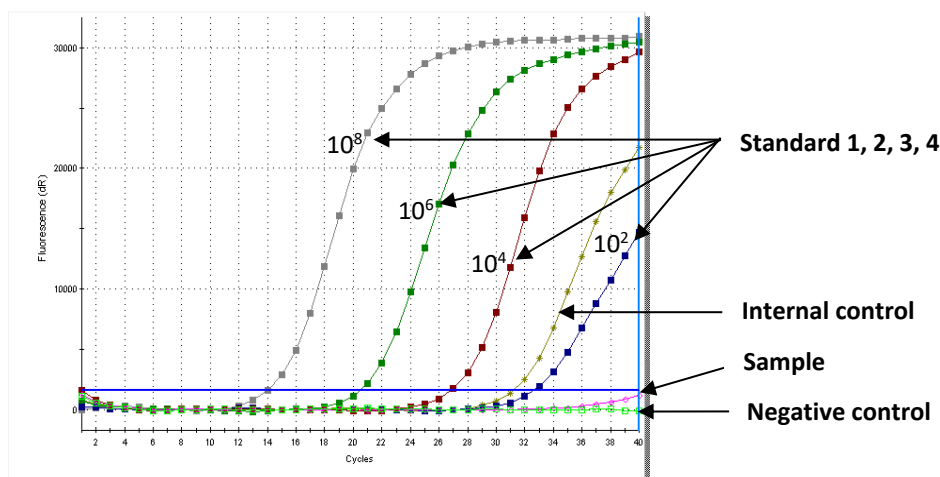

3. CONCLUSION:

The viral load: ≤ 2.40 \log_{10}
 The viral load: ≤ 50 IU/ml
 The viral load: ≤ 250 copies/ml

Limit of detection

$\leq 2.40 \log_{10}$
 ≤ 50 IU/mL
 ≤ 250 Copies/ml

CHARGE OF LAB



MA. NGUYEN THUY DA THAO