

ID No: 00220122023

TEST RESULT SHEET


Date 20 month 12 year 2023

1. SAMPLE INFORMATION:

Patient name: **CHANG KHENG ENG** Sex: **Female** Age: **55**
 Testing requirements: **HBV-DNA Quantitative**
 Address: **BIOKHON LAB**
 Test technique: **Real-time PCR – Photomultiplier Tube Technique**
The FAM labeled probe to detect the target DNA
The HEX labeled probe to detect the Internal control

2. RESULTS:

Amplification Plots

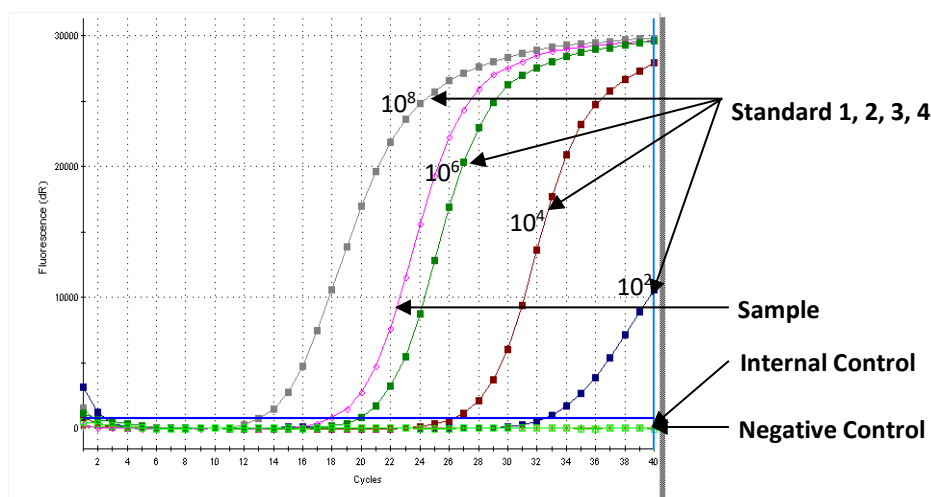

3. CONCLUSION:

The viral load: 8.27	\log_{10}	$\leq 2.40 \log_{10}$
The viral load: 37,299,008	IU/ml	$\leq 50 \text{ IU/mL}$
The viral load: 186,495,038	copies/ml	$\leq 250 \text{ Copies/ml}$

Limit of detection

CHARGE OF LAB



MA. NGUYEN THUY DA THAO