



CHANG
KHENG ENG
F
01/01/1970


Height: 160 cm
Weight: 54.0 kg
Physician: Chronic hepatitis B
Fasting: No

CAP (dB/m)		E (kPa)
IQR	MEDIAN	MEDIAN
18	206	19.2
		IQR/Med 17%

21/12/2023 10:17:59
Exam: M
SWF = 50Hz
Organ: Liver
Operator: OENG LEANGSENG
E-MEASUREMENTS: 10

liver stiffness is 19.2KPa which equal F4 on the METAVIR score.

Dr. OENG LEANGSENG

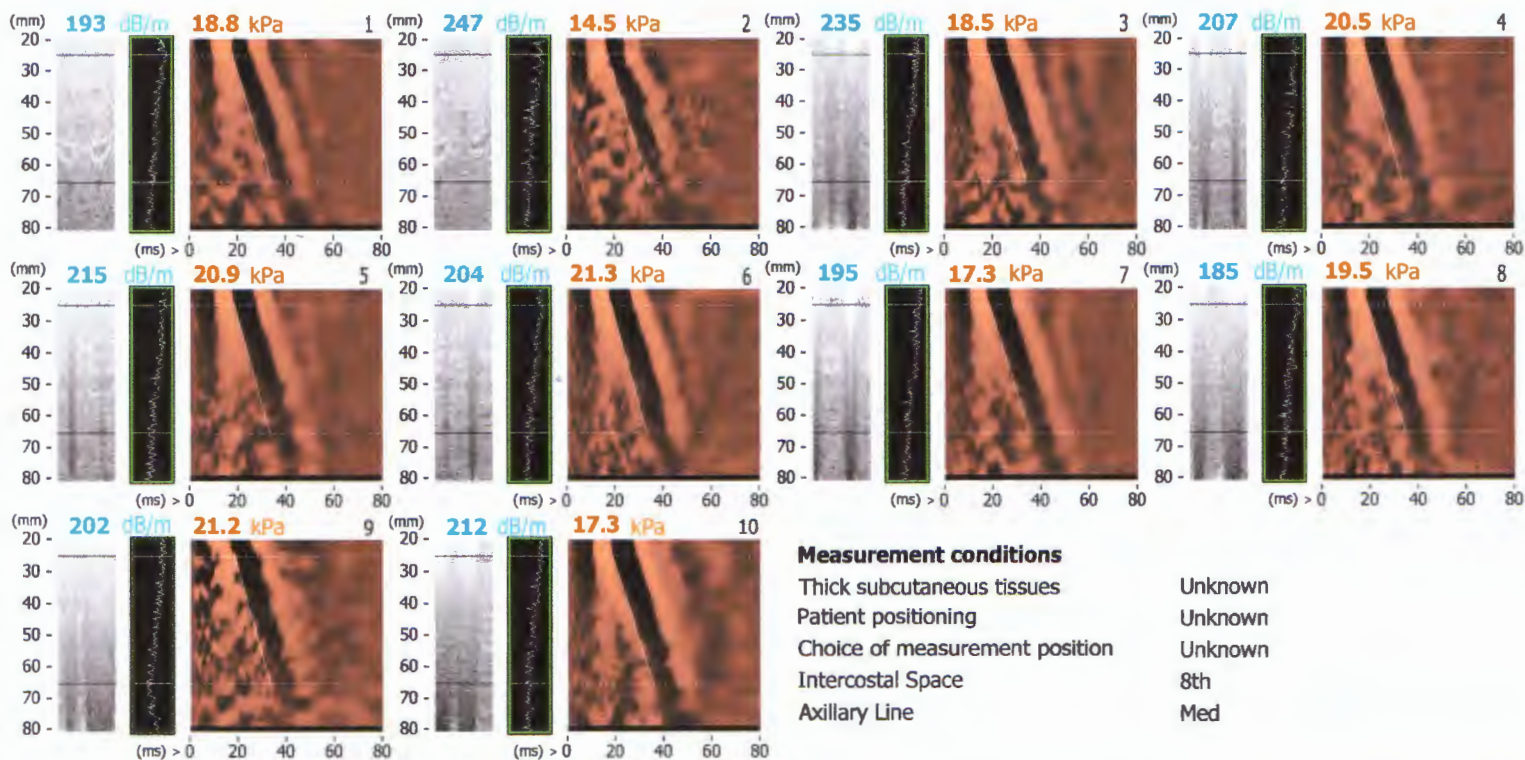

Measurement conditions

Thick subcutaneous tissues
Patient positioning
Choice of measurement position
Intercostal Space
Axillary Line

Unknown
Unknown
Unknown
8th
Med

FibroScan 530 Compact / SN: F82067 Probe M+ / SN: 2002382 Software release number FS 4.1.3

FibroScan® is a medical device intended as an aid for the management of patients with liver disease. Measurements should be performed by a certified operator. The values obtained must be interpreted by a physician experienced in dealing with liver disease, taking into account the complete medical records of the patient, the number of valid measurements and their dispersion. Probes must be calibrated according to the manufacturer's recommendations.