

ID No: 00102102023

TEST RESULT SHEET


Date 02 month 10 year 2023

1. SAMPLE INFORMATION:

Patient name: **HENG CHAM NOL** Sex: **Male** Age: **61**
 Testing requirements: **HCV-RNA Quantitative**
 Address: **BIOKHON LAB**
 Test technique: **Real-time PCR – Photomultiplier Tube Technique**
The FAM labeled probe to detect the target DNA
The HEX labeled probe to detect the Internal control

2. RESULTS:

Amplification Plots

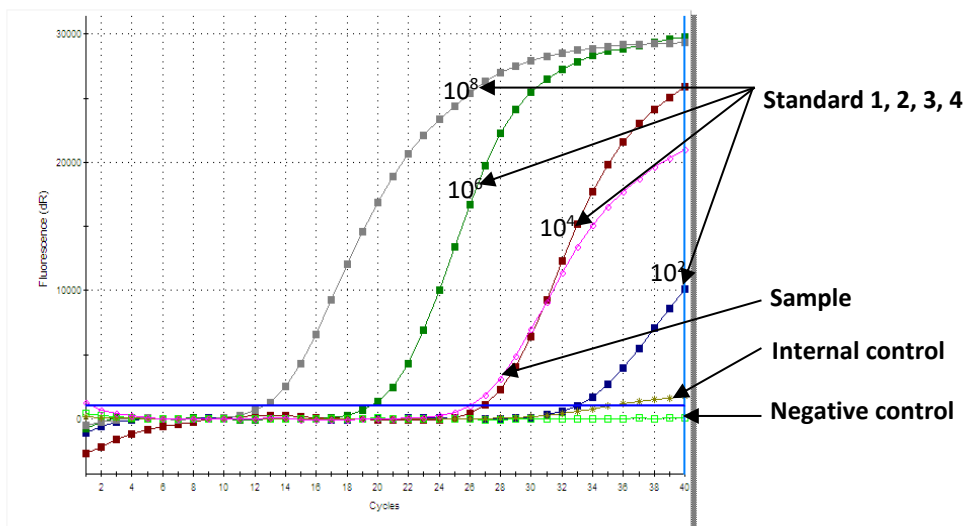

3. CONCLUSION:

The viral load: 5.80
 The viral load: 126,909
 The viral load: 634,545

\log_{10}
 IU/ml
 copies/ml

Limit of detection

$\leq 2.40 \log_{10}$
 $\leq 50 \text{ IU/mL}$
 $\leq 250 \text{ Copies/mL}$

CHARGE OF LAB



MA. NGUYEN THUY DA THAO