



Calmette Hospital
Gastrointestinal
Phnom Penh



លេខ..... កម្ម.២០

KOY
SOREN
M
06/04/1969


Height: 175 cm
Weight: 71.0 kg
Physician:
Chronic hepatitis B
Fasting: Unknown

	CAP (dB/m)	E (kPa)
	IQR	MEDIAN
	40	196 5.9
	0.5	IQR/Med
	8%	

21/10/2024 13:02:29

Exam: M
Uncalibrated probe
SWF = 50Hz
Organ: Liver
Operator: Operator
E-MEASUREMENTS: 10

LIVER stiffness is 5.9kpa equal to F0-F1

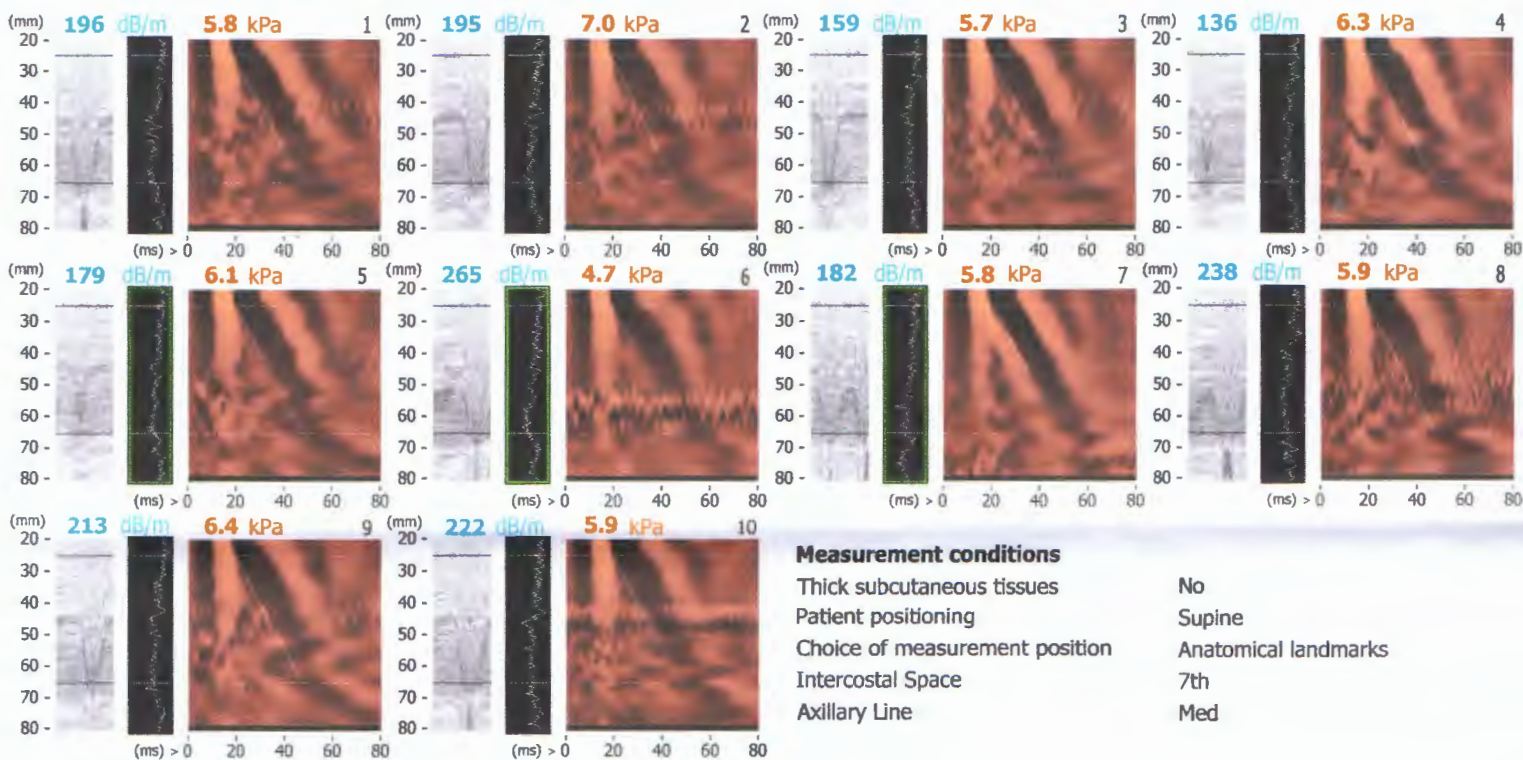

Measurement conditions

Thick subcutaneous tissues
Patient positioning
Choice of measurement position
Intercostal Space
Axillary Line

No
Supine
Anatomical landmarks
7th
Med

FibroScan 530 Compact / SN: F82067 Probe M+ / SN: 2002382 Software release number FS 4.1.3

FibroScan® is a medical device intended as an aid for the management of patients with liver disease. Measurements should be performed by a certified operator. The values obtained must be interpreted by a physician experienced in dealing with liver disease, taking into account the complete medical records of the patient, the number of valid measurements and their dispersion. Probes must be calibrated according to the manufacturer's recommendations.

